


## MAIN FEATURES

- LATEX ENHANCED IMMUNOTURBIDIMETRIC METHOD
- EASY TO PROGRAM ON ANY TYPE OF AUTOMATED ANALYZERS
- GOOD CORRELATION WITH A ELISA COMMERCIAL PROCEDURE
- RANGE OF ANALYSIS.....0.0 – 1 200 MG/L
- GOOD PRECISION.....INTER-RUN: CVs < 4.7 %  
.....INTRA-RUN: CVs < 5.1 %
- LIQUID REAGENTS .....READY TO USE
- SELF-LIFE.....2 YEARS
- PROZONE .....> 2 250 MG/L
- LDD .....< 5 MG/L

## GENERAL APPLICATION

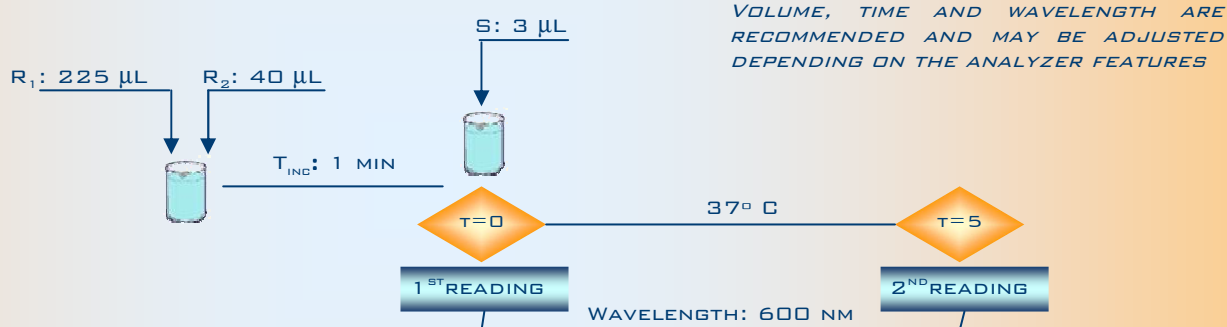

## PRECISION

(\*) LEAST DETECTABLE DOSE (SENSITIVITY) DETERMINED AS THE LIPOPROTEIN (A) CONCENTRATION NEEDED FOR A THREE DEVIATION RESPONSE OVER THE 0.0 MG/L STANDARD ONE

CONTROL	LEVEL 1	LEVEL 2	LEVEL 3
MEAN MG/L	160	479	715
SD	7.52	21.50	24.31
CV %	4.7	4.5	3.4

WITHIN-RUN PRECISION (N=10)

CONTROL	LEVEL 1	LEVEL 2	LEVEL 3
MEAN MG/L	160	479	715
SD	8.41	18.09	25.20
CV %	5.1	3.9	3.5

BETWEEN-RUN PRECISION (N=10)

## SENSITIVITY\*

CONTROL	LEVEL 1
N	20
LDD MG/L	<5.0


SENSITIVITY

## ORDER INFORMATION


ANOTHER PRESENTATIONS ARE AVAILABLE ON REQUEST

- REF: K-9520T LIPOPROTEIN (A) BUFFER ..... 30 ML
- REF: S-9320T LIPOPROTEIN (A) LATEX ..... 4 ML
- REF: C-9320T LIPOPROTEIN (A) CALIBRATOR ..... 1 ML (LYOPH.)
- REF: G-9320T LIPOPROTEIN (A) CONTROL LOW ..... 1 ML (LYOPH.)


## CALIBRATION CURVE

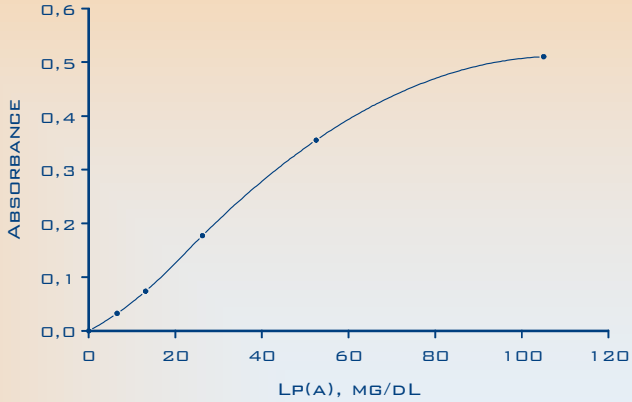

## PROZONE

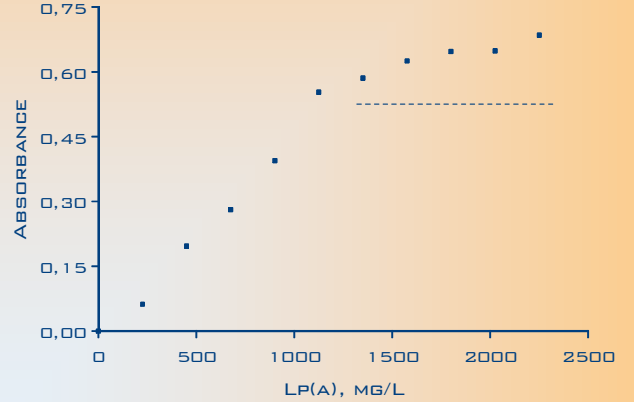

## METHOD COMPARISON

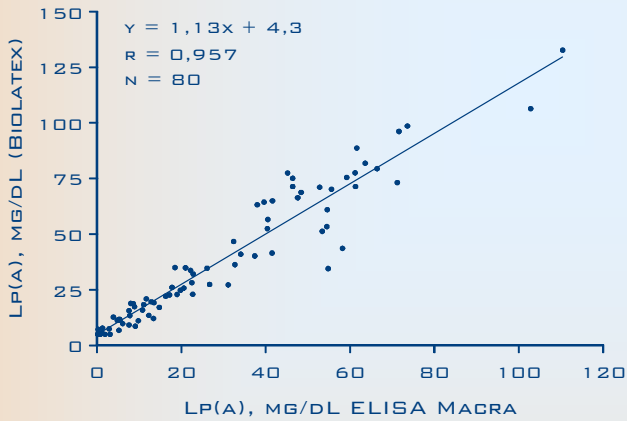

## LINEARITY

