


MAIN FEATURES

- LATEX ENHANCED IMMUNOTURBIDIMETRIC MONOREAGENT METHOD
- EASY TO PROGRAM ON ANY TYPE OF AUTOMATED ANALYZERS
- GOOD CORRELATION WITH A COMMERCIAL PROCEDURE
- RANGE OF ANALYSIS.....0.0 – 800 MG/L
- GOOD PRECISION.....INTER-RUN: CVs < 4.42 %
.....INTRA-RUN: CVs < 4.76 %
- LIQUID REAGENTSREADY TO USE
- SELF-LIFE2 YEARS
- PROZONE> 2200 MG/L
- LDD< 15 MG/L

GENERAL APPLICATION

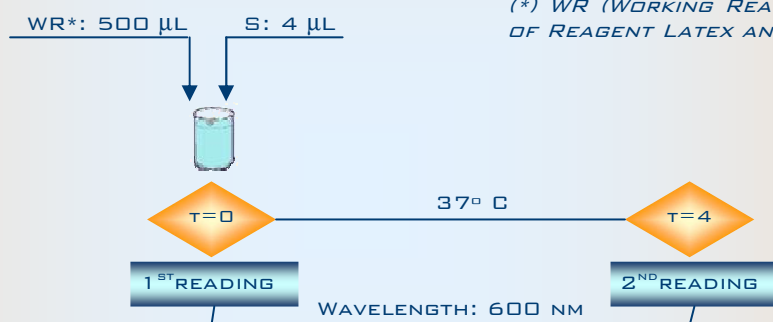

(* WR (WORKING REAGENT) IS PREPARED MIXING ONE PART OF REAGENT LATEX AND SEVEN PARTS OF REAGENT BUFFER

PRECISION

(* LEAST DETECTABLE DOSE (SENSITIVITY) DETERMINED AS THE LIPOPROTEIN (A) CONCENTRATION NEEDED FOR A THREE DEVIATION RESPONSE OVER THE 0.0 MG/L STANDARD ONE

LEVEL	1	2	3
N	10	10	10
CONCENTRATION MG/L	90	170	325
CV %	1.74	1,97	4.42

INTRA-ASSAY PRECISION

LEVEL	1	2	3
N	10	10	10
CONCENTRATION MG/L	90	170	325
CV %	3.27	1.70	4.76

INTER-ASSAY PRECISION

SENSITIVITY*

CONTROL	LEVEL 1
N	20
LDD MG/L	< 15.0


SENSITIVITY

ORDER INFORMATION


ANOTHER PRESENTATIONS ARE AVAILABLE ON REQUEST

- REF: K-9520M LIPOPROTEIN (A) BUFFER 45.5 ML
LIPOPROTEIN (A) LATEX 6.5 ML
LIPOPROTEIN (A) CALIBRATOR 1 ML (LYOPH.)
- REF: C-9320T LIPOPROTEIN (A) CONTROL 1 ML (LYOPH.)


CALIBRATION CURVE

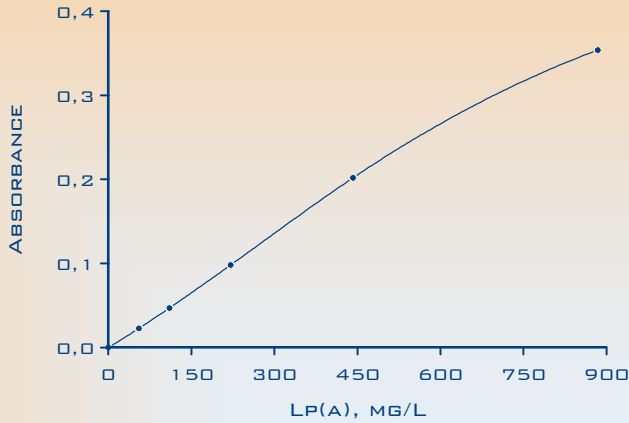

PROZONE

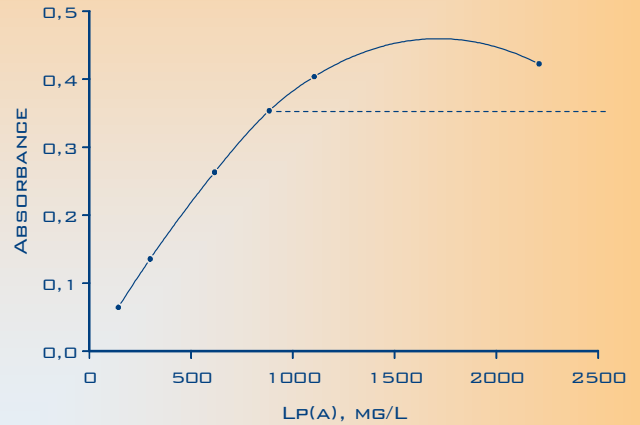

METHOD COMPARISON

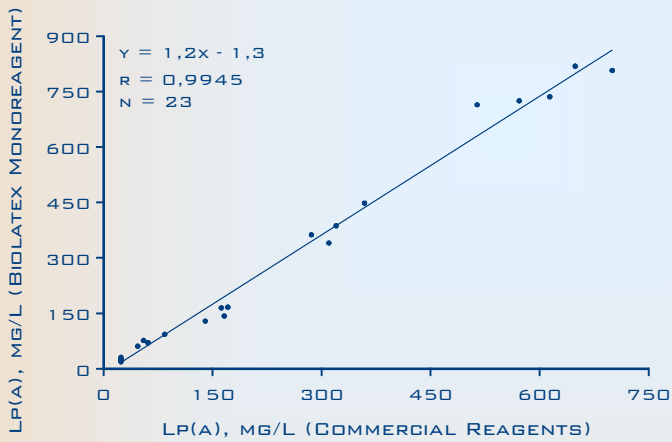

LINEARITY

